Righteous Research

PO Box 582
Kahului, HI 96733

krause analytical

COC# 145948
Lab # 214919
Date Rec'd 9/29/2026
Report Issued 10/8/2026

Certificate of Analysis



Project
Compound Retatrutide
Label Claim 15 mg
Batch/Lot SQ09082026

Analyte	Result	Units	LOQ	% of Label	Method	Date	CAS
Peptides & Bioactives							
Chromatographic purity	>99.9	%	1		HPLC-UV/MS	10/1/2026	
Retatrutide	13.7	mg	.1	91.3	HPLC-UV-MS	10/1/2026	2381089-83-2
Mass Spectral Match	ID Confirmed				HPLC-UV-MS	10/1/2026	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Data is not for regulatory compliance nor diagnostic use.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
OCH - above calibrated range OCL - below calibrated range
All values reported on a per vial basis unless otherwise noted
Copyright © 2026 Krause Analytical LLC. All rights reserved.

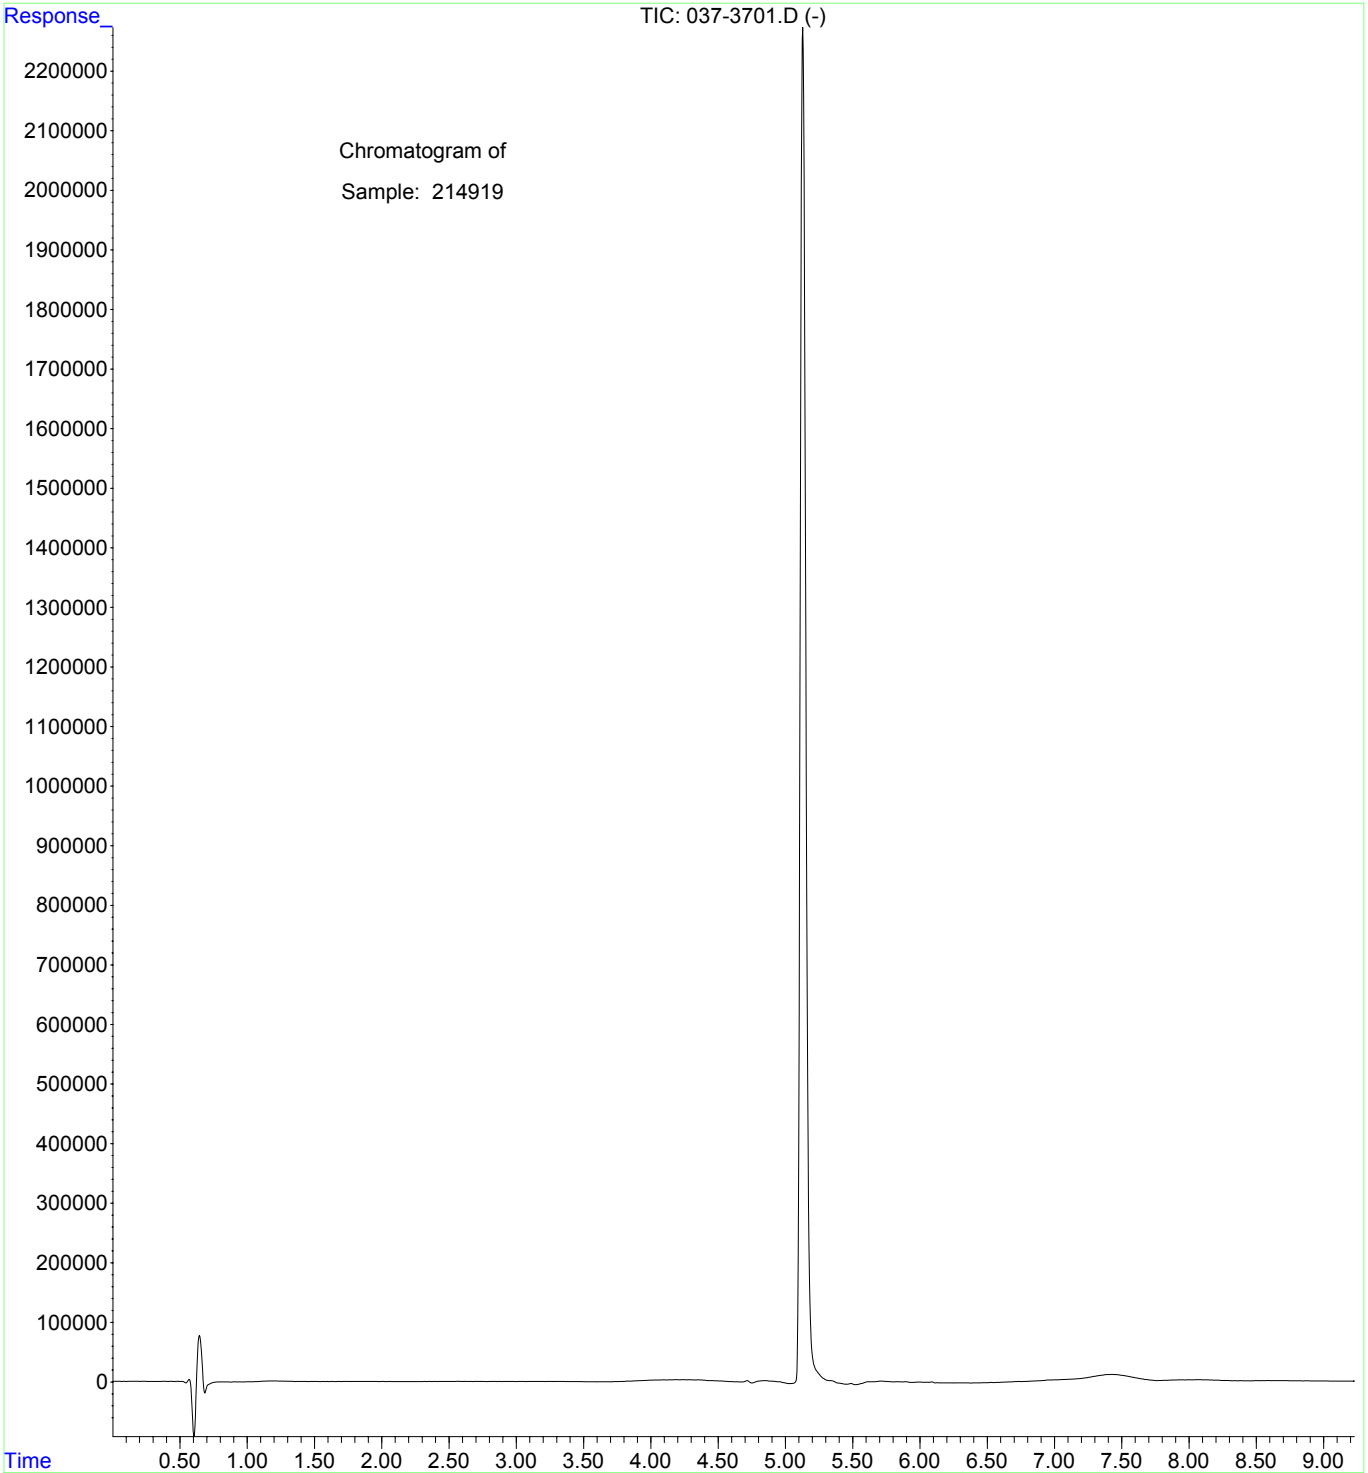
Respectfully submitted,

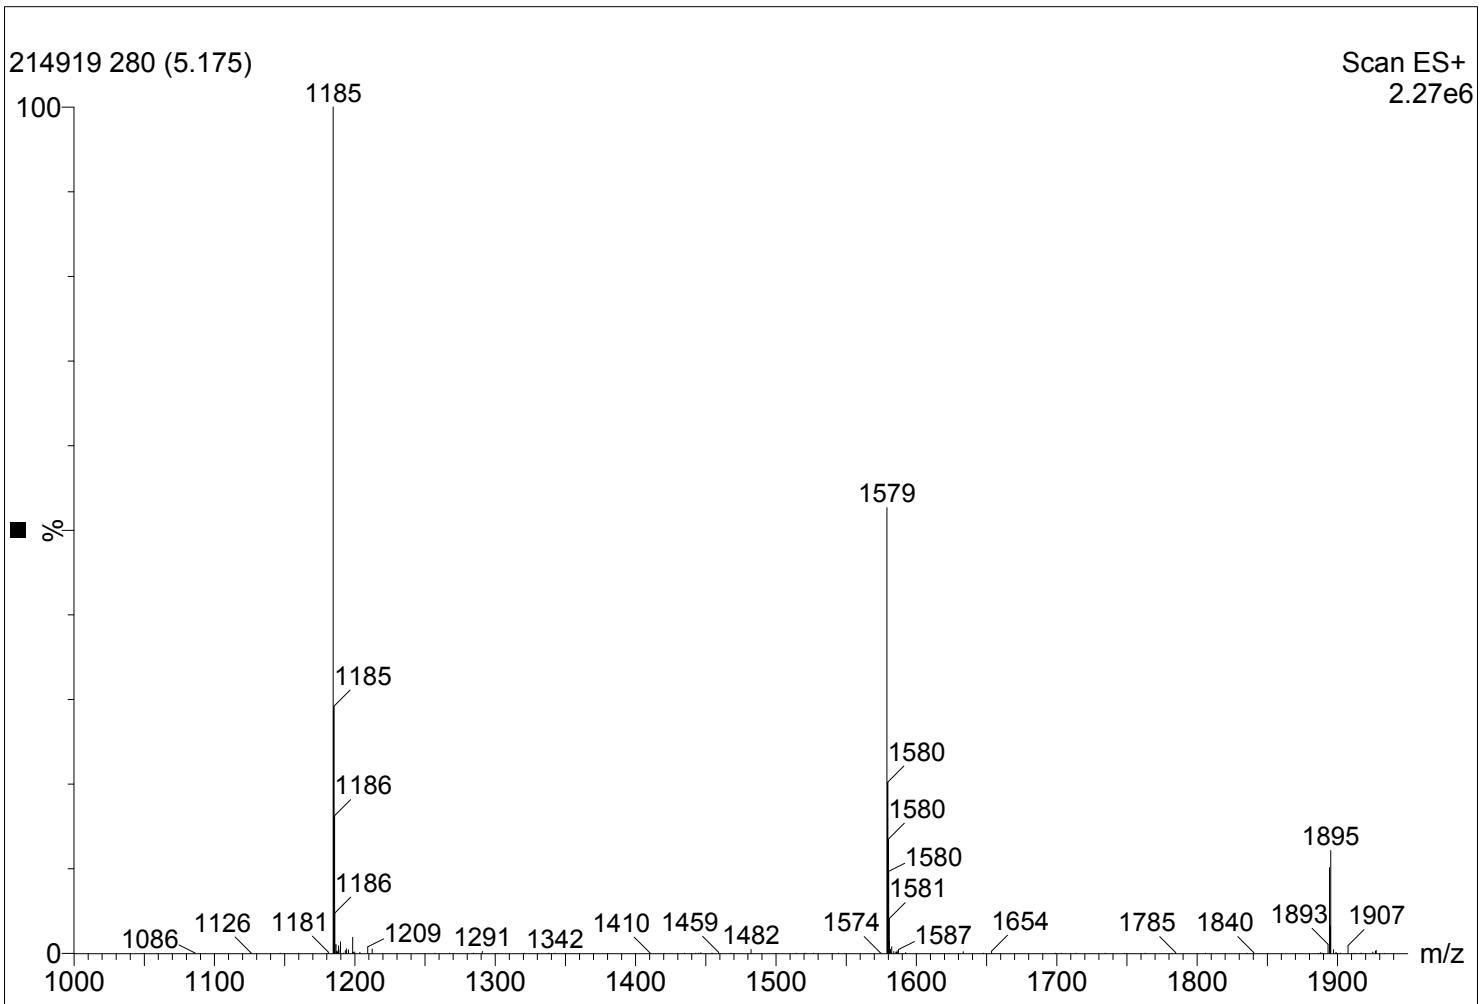
Mark C. Krause
Laboratory Director

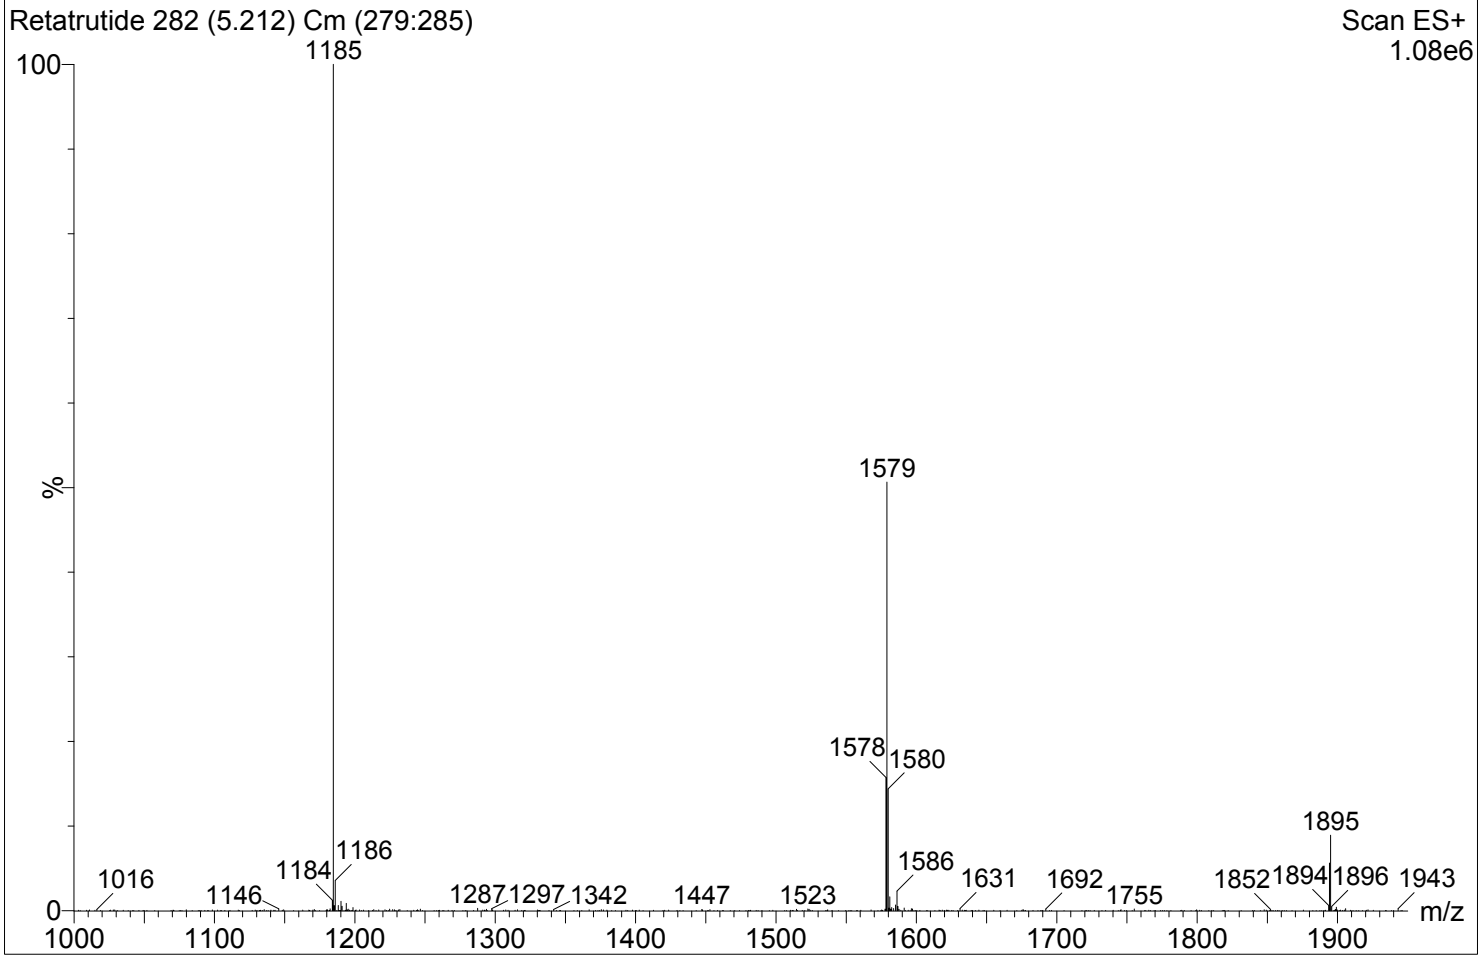
****

CHROMATOGRAM

****




214919 280 (5.175)
Scan ES+
2.27e6
100
%
0
1185
1579
1185
1186
1186
1580
1580
1580
1581
1895
1086
1126
1181
1209
1291
1342
1410
1459
1482
1574
1587
1654
1785
1840
1893
1907
1000
1100
1200
1300
1400
1500
1600
1700
1800
1900
m/z


Retatrutide 282 (5.212) Cm (279:285)
Scan ES+
1.08e6
100
%
0
1185
1579
1578
1580
1184
1186
1586
1895
1016
1146
1287
1297
1342
1447
1523
1631
1692
1755
1852
1894
1896
1943
1000
1100
1200
1300
1400
1500
1600
1700
1800
1900
m/z