Righteous Research

PO Box 582
Kahului, HI 96733

krause analytical

COC# 145948
Lab # 214918
Date Rec'd 9/29/2026
Report Issued 10/8/2026

Certificate of Analysis



Project
Compound Tirzepatide
Label Claim 30 mg
Batch/Lot SQ09082026

Analyte	Result	Units	LOQ	% of Label	Method	Date	CAS
Peptides & Bioactives							
Chromatographic purity	>99.9	%	1		HPLC-UV/MS	10/2/2026	
Tirzepatide	29.2	mg	.1	97.4	HPLC-UV-MS	10/2/2026	2023788-19-2
Mass Spectral Match	ID Confirmed				HPLC-UV-MS	10/2/2026	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Data is not for regulatory compliance nor diagnostic use.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
OCH - above calibrated range OCL - below calibrated range
All values reported on a per vial basis unless otherwise noted
Copyright © 2026 Krause Analytical LLC. All rights reserved.

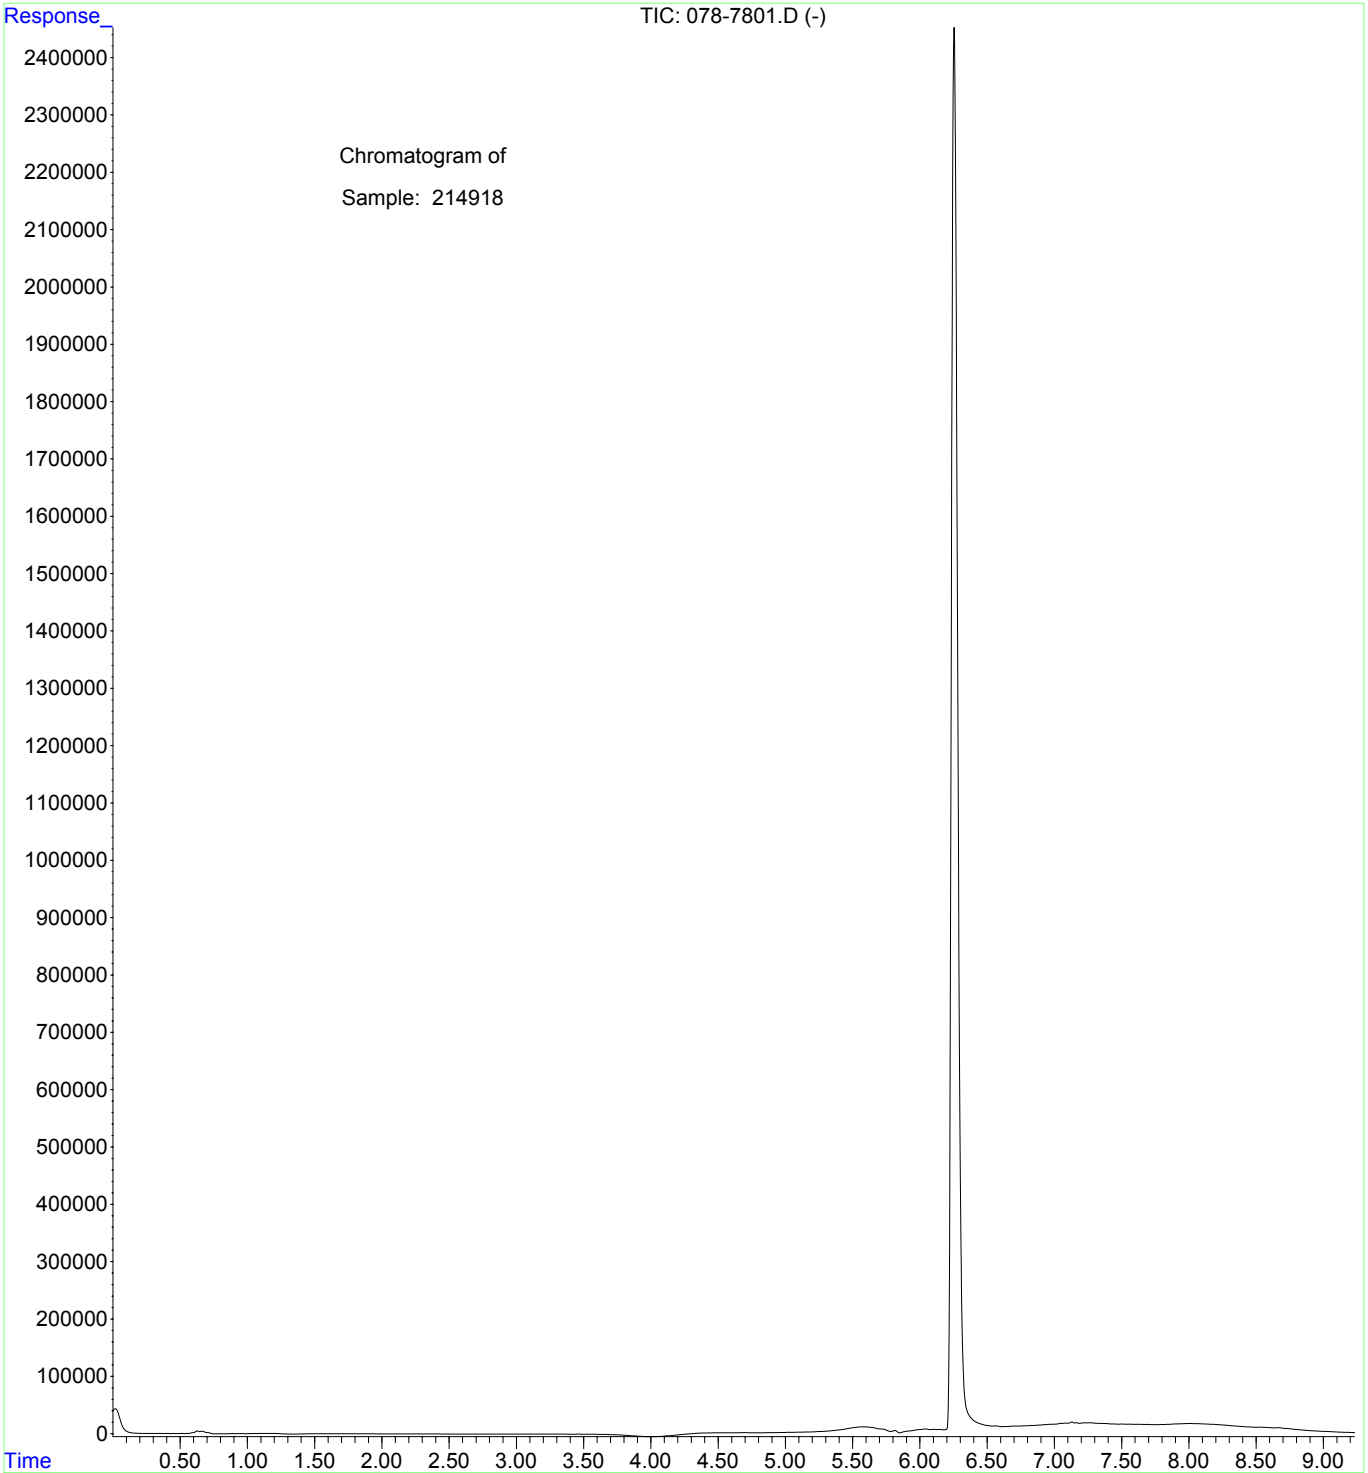
Respectfully submitted,

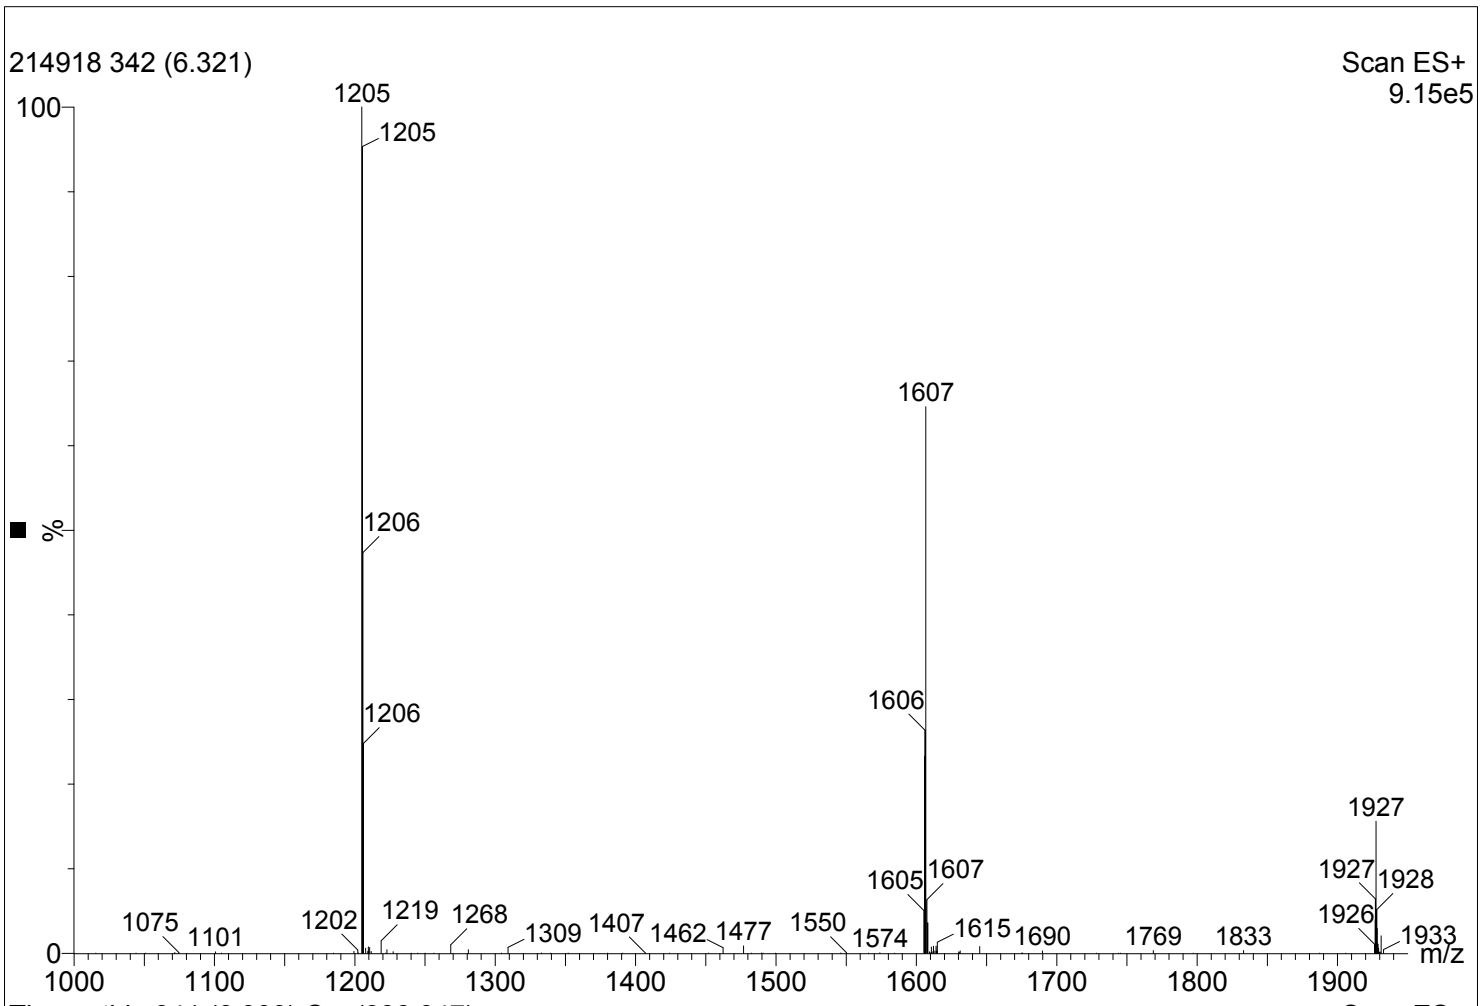
Mark C. Krause
Laboratory Director

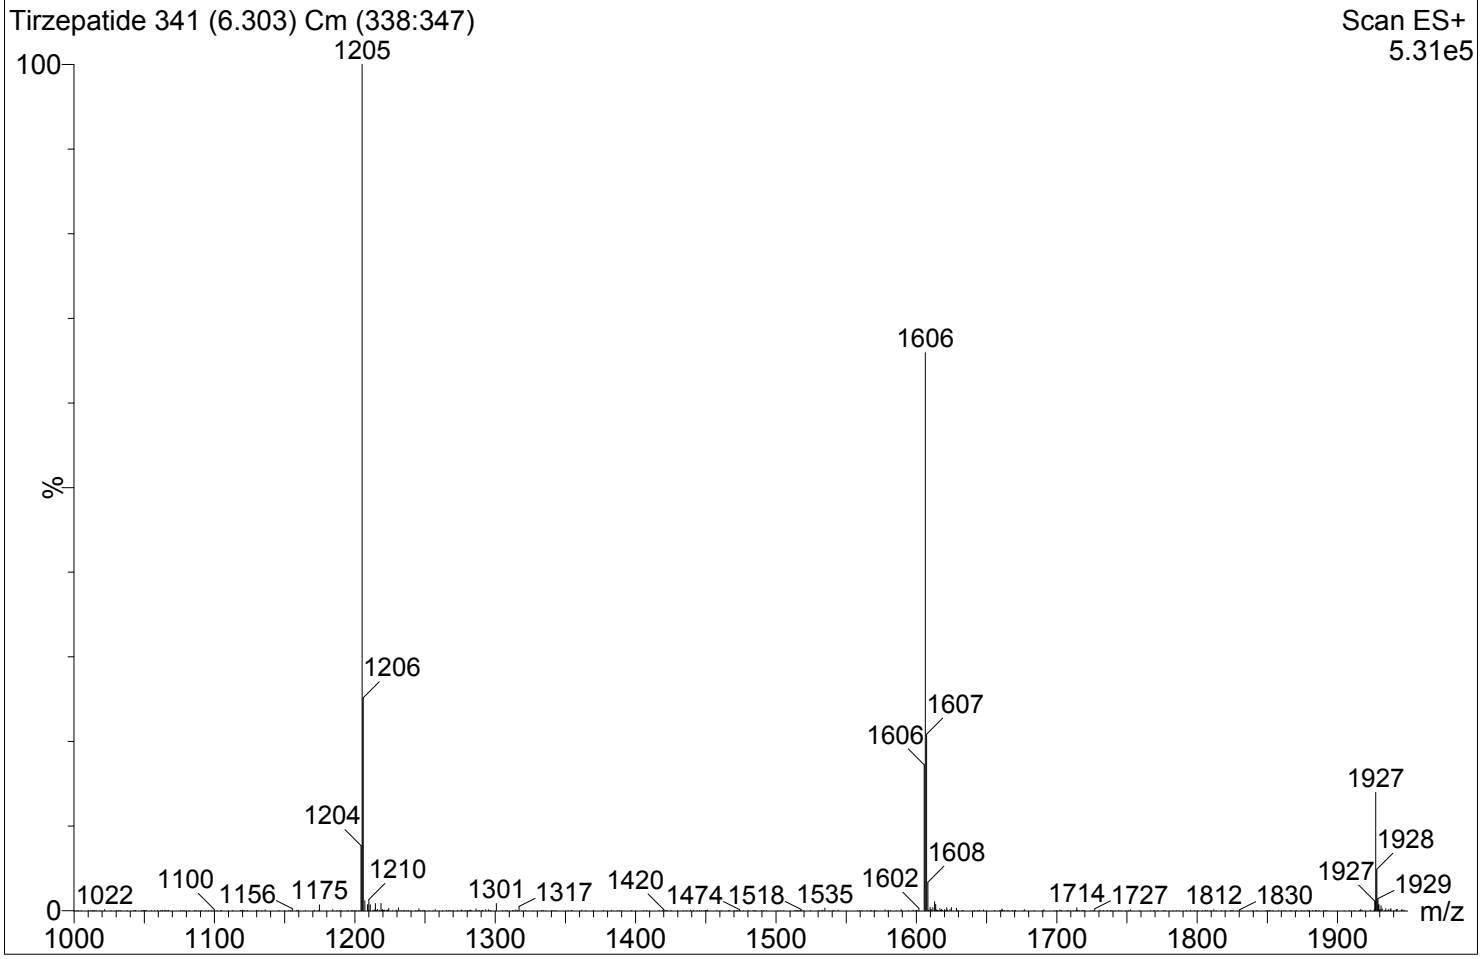
****

CHROMATOGRAM

****




214918 342 (6.321)
Scan ES+
9.15e5
100
%
0
1205
1205
1607
1206
1606
1206
1927
1605
1607
1927
1928
1926
1075
1101
1202
1219
1268
1309
1407
1462
1477
1550
1574
1615
1690
1769
1833
1933
m/z
1000
1100
1200
1300
1400
1500
1600
1700
1800
1900


Tirzepatide 341 (6.303) Cm (338:347)
Scan ES+
5.31e5
100
%
0
1205
1606
1206
1607
1606
1927
1204
1928
1608
1927
1210
1929
1022
1100
1156
1175
1301
1317
1420
1474
1518
1535
1602
1714
1727
1812
1830
m/z
1000
1100
1200
1300
1400
1500
1600
1700
1800
1900